
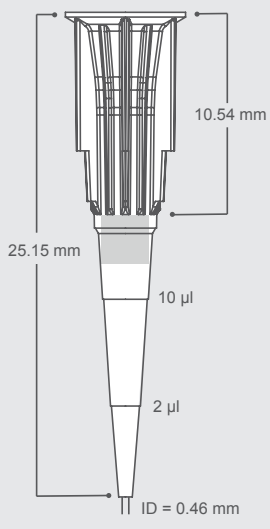


M-0010-9FC

M-0010-9SC

Description	10 µl Filter Tip	10 µl Tip
Biotix Part #	M-0010-9FC	M-0010-9SC
Maximum volume	10 µl	10 µl
Graduation marks	Yes	Yes
Certified Sterile and free of key contaminants	Yes	Yes
Material	Clear polypropylene	Clear polypropylene
Packaging	96 tips per rack, 10 racks per pack, 5 packs per case	96 tips per rack, 10 racks per pack, 5 packs per case
X-Resin	Yes	Yes
FlexFit	Yes	Yes
Blade	Yes	Yes
Delta Filter	Yes	No
Technical Drawings		

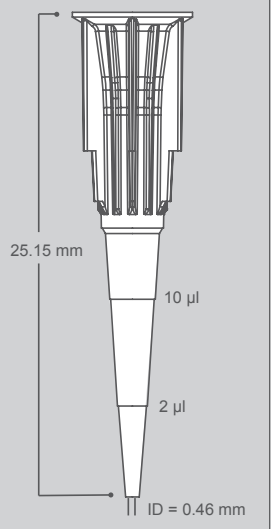

Quality Testing:

RNase/ DNase	Products are washed in distilled water and concentrated via centrifugation. Samples are added to previously established nucleic acid standards, incubated for one hour at 37°C, and tested on a 2% gel using electrophoresis. Products must show no degradation of standards to pass. Test sensitivity is 10 ⁻⁷ Kunitz units/μl.
Nucleic Acid	Products are washed in distilled water and concentrated via centrifugation. Then, samples are added to protocol specified PCR reactions and thermal cycled for 50 cycles. A 2% agarose gel electrophoresis is used to examine experimental samples, positive controls, and negative controls. To pass, product samples must show no DNA amplification. Test sensitivity is 10 ng.
Endotoxin/ Pyrogen	Products are tested for endotoxins by using the Limulus Amebocyte Lysate (LAL) gel assay according to FDA guidelines. Test sensitivity is 0.06 EU/ml.
Trace Metal	Products are washed in distilled water. The sample is then tested using reflectometry using a single strip test for the following metals: Ca, Cu, Fe, K, Mg, Mn and Ni. Standard solutions are used as positive controls. A reader is used to detect metals to a sensitivity of 500 mg/L.
PCR Inhibitor	Products are tested via PCR amplification and gel electrophoresis analysis. Samples must show normal amplification to be considered free of PCR inhibitors.
Sterilization	Products are sterilized using electron beam irradiation.
CV Test	Each lot of Biotix product is CV tested and the resulting CV is then printed on the pack label. The volume tested is equal to the maximum volume per tip size.
TIR-Total Indicated Runout	Biotix pipette tips are tested to ensure that they meet the SBS standards. Individual products specify their compatibility with 96, 384 or 1536-well plates.

Proprietary Technologies:

FlexFit	Ergo design Patents Pending
X-Resin	Proprietary resin, virgin polypropylene
Delta Filter	Color change filter Patents Pending
Blade	Minimal distal end orifice Patents Pending

Pipettor Compatibility:

Biohit Proline™ 10 μl

Brand Transferpette S™ 10 μl

Capp™ 10 μl

CLP Beta-Pette™ 2 μl and 10 μl

CLP Poseidon™ 2 μl and 10 μl

CLP Poseidon Electronic™ 20 μl

Eppendorf Reference™ 2.5 μl
(works with M-0010-9SC)

Eppendorf Reference™ 10 μl

Eppendorf Research™ 2.5 μl
(works with M-0010-9SC)

Eppendorf Research™ 10 μl

Eppendorf Research Plus™ 2.5 μl
(works with M-0010-9SC)

Eppendorf Research Plus™ 10 μl

Eppendorf Xplorer™ 10 μl

Finnpipette™ 10 μl and 50 μl

Finnpipette™ Electronic 10 μl

Finnpipette F1™ 10 μl

Gilson Pipetman™ P2 and P10

Hamilton™ 2 μl and 10 μl

Nichiryo Nichipet EX™ 10 μl

Nichiryo Oxford Benchmate™ 2 μl

Nichiryo Oxford Multimate™ 10 μl

Socorex Calibri 822™ 10 μl

VWR Ultra High Performance™
2 μl and 10 μl